

Quick Start Guide

Moxi GO II

Before you Begin:

Your Moxi GO II comes with a partial battery charge and must be run plugged into the supplied power adapter for charging and running tests.

Required Materials:

- Cassettes and diluent (e.g. PBS).
- Biological cell sample.
- Pipette and tips for 60µL aliquot.

Cassette Specifications:

- Cassette size range: 3 - 26µm particles
- Concentration range:
 - * Counts: 10,000 to 1,750,000 cells/ml
 - * Optimal Fluorescence Sensitivity: 100,000 - 500,000 cells/ml

Sample Prep Considerations:

- **Solution Conductivity:** Cells must be suspended in 0.9% salt solution (e.g. PBS or equivalent) for proper sizing and test function.
- **Single-Cell Suspensions:** Cells need to be prepared as single cell suspensions. Clusters/aggregates should be broken apart with mechanical trituration and/or protease dissociation (e.g., Accutase). Samples with large extracellular debris particles or aggregates should be strained/filtered before running.
- **Fluorescent Labeling/Stains:** The Moxi GO II uses a 488nm laser with 525/45nm (e.g. FITC) and EITHER 561nm LP (e.g. R-PE, PI, 7-AAD, PE-Cy5) OR ~650nm/LP (e.g. PI, PE-Cy5) emission filters.
- ORFLO approved/kits reagents, and protocols are strongly recommended.

Data Transfer:

FCS 3.1 test data is available for transfer via USB. Just plug the unit into a PC/Mac with supplied cable. The unit will appear as an external, flash drive.

User Manual:

An electronic copy of the complete Moxi GO II user manual can be found at www.ORFLO.com by following the "Resources" and then "User Manuals" links.


1) Turn Moxi GO II ON



4) Auto Laser Alignment. Please Wait.




2) Touch Desired Assay

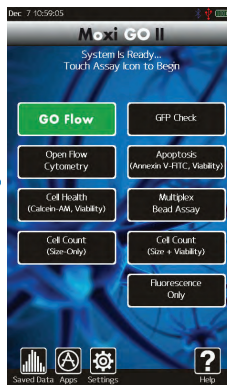

5) Pipette 60µL of Stained Sample Into the Cassette. Close Door. Test Begins.




3) Open the Door. Depress Black Knob Fully. Insert Cassette. Release Knob.



8) Data Summary



- Application
- PMT Displayed
- Cell % Results
- Greyed Noise Region
- Toggle to Angle Gate
- Fluorescent Gain Setting
- Lower Gated Population Results
- Press to Change Size Scale Range: 2-26, 2-18, 2-10 µm

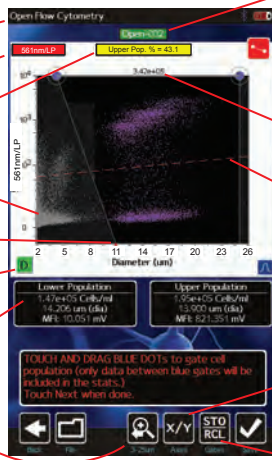

- Touch to Rename File
- Battery/Charging Indicator
- Toggle Between Size (Blue) and Fluorescent (Red) and Noise (Yellow) Gates.
- Total Count Between Size (blue) Gates
- Fluorescent Gate (Red)
- Turn on Histogram Overlays
- Upper Gated Population Results
- Select to Change Axis Display: PMT vs Size, Size/Fluorescence Histograms, PMT vs PMT
- Store/Recall Gate Locations

Dot Plot Results


Opening Viewing Comparing, and Printing Data:

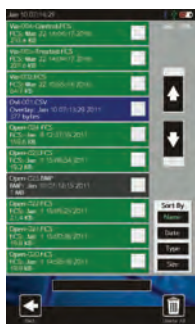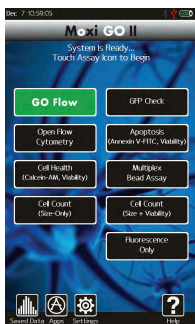


Touch and drag gates to adjust

Touch red icon to toggle gate modes

Specify y-axis parameter

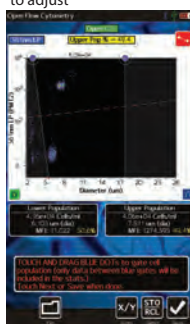

X/Y

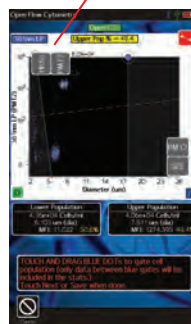

Specify x-axis parameter




Test Comparisons/Overlays



STO RCL

HOLD SIZE

HOLD PMT2

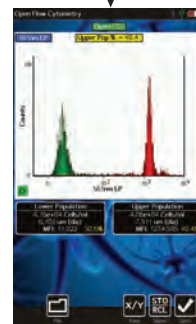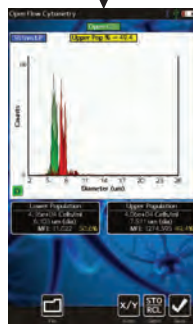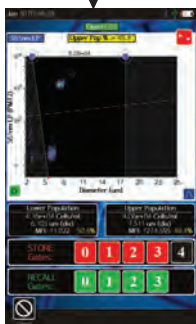



Touch number to store/recall gates into/from memory



Print Screen (export to .bmp file)

Use blue size gates to define region to be compared

Compare Overlay Tests

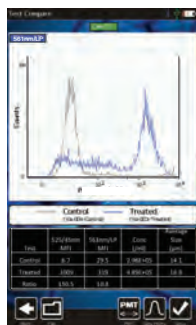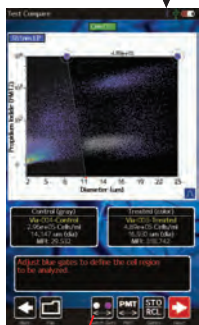

"Switch Sets" toggles the "control" and "treated" set designations



Exact screenshot saved as a .bmp file on the data disk (access through USB connection to the computer)